

1/3

BASELINE AND 120 MINUTES POST-TREATMENT VISCOSITY MEASUREMENTS

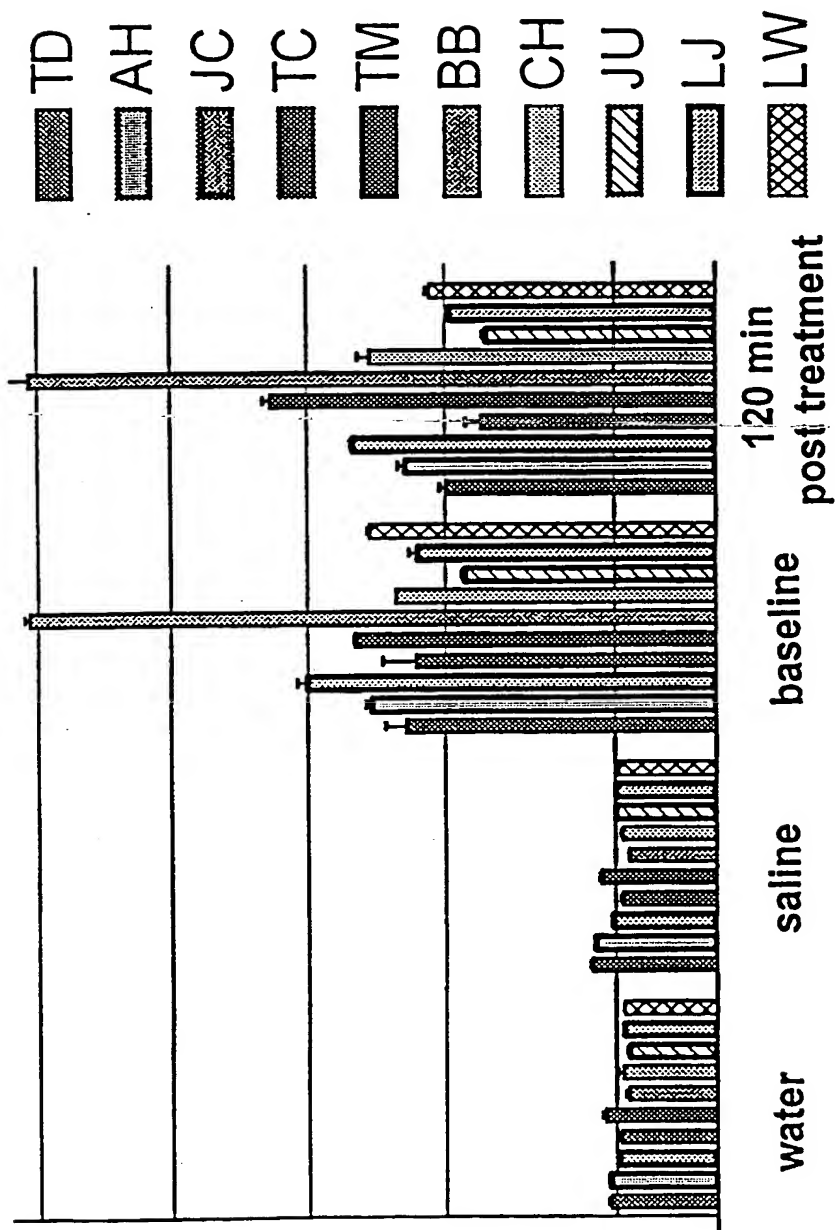


Fig. 1

CONTROL IN VITRO VISCOSITY

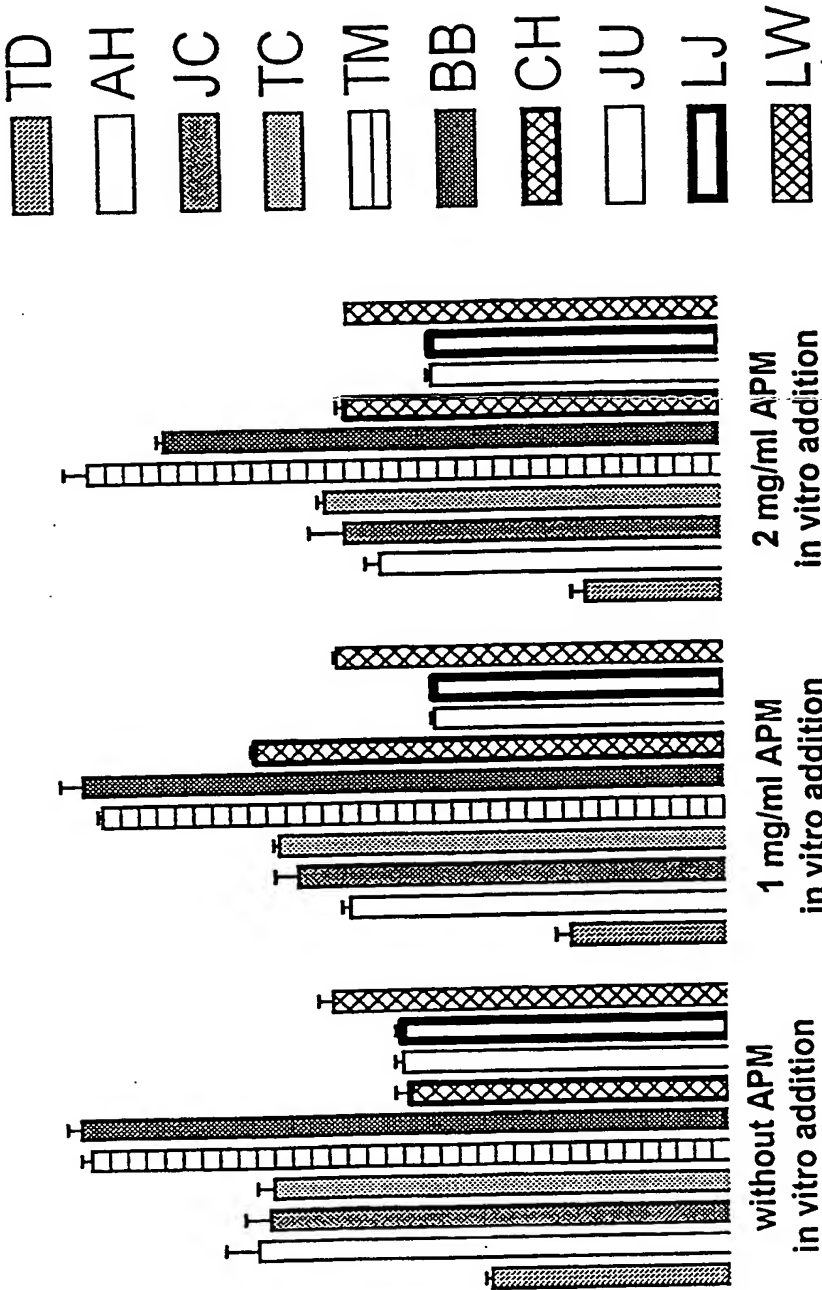


Fig. 2

3/3

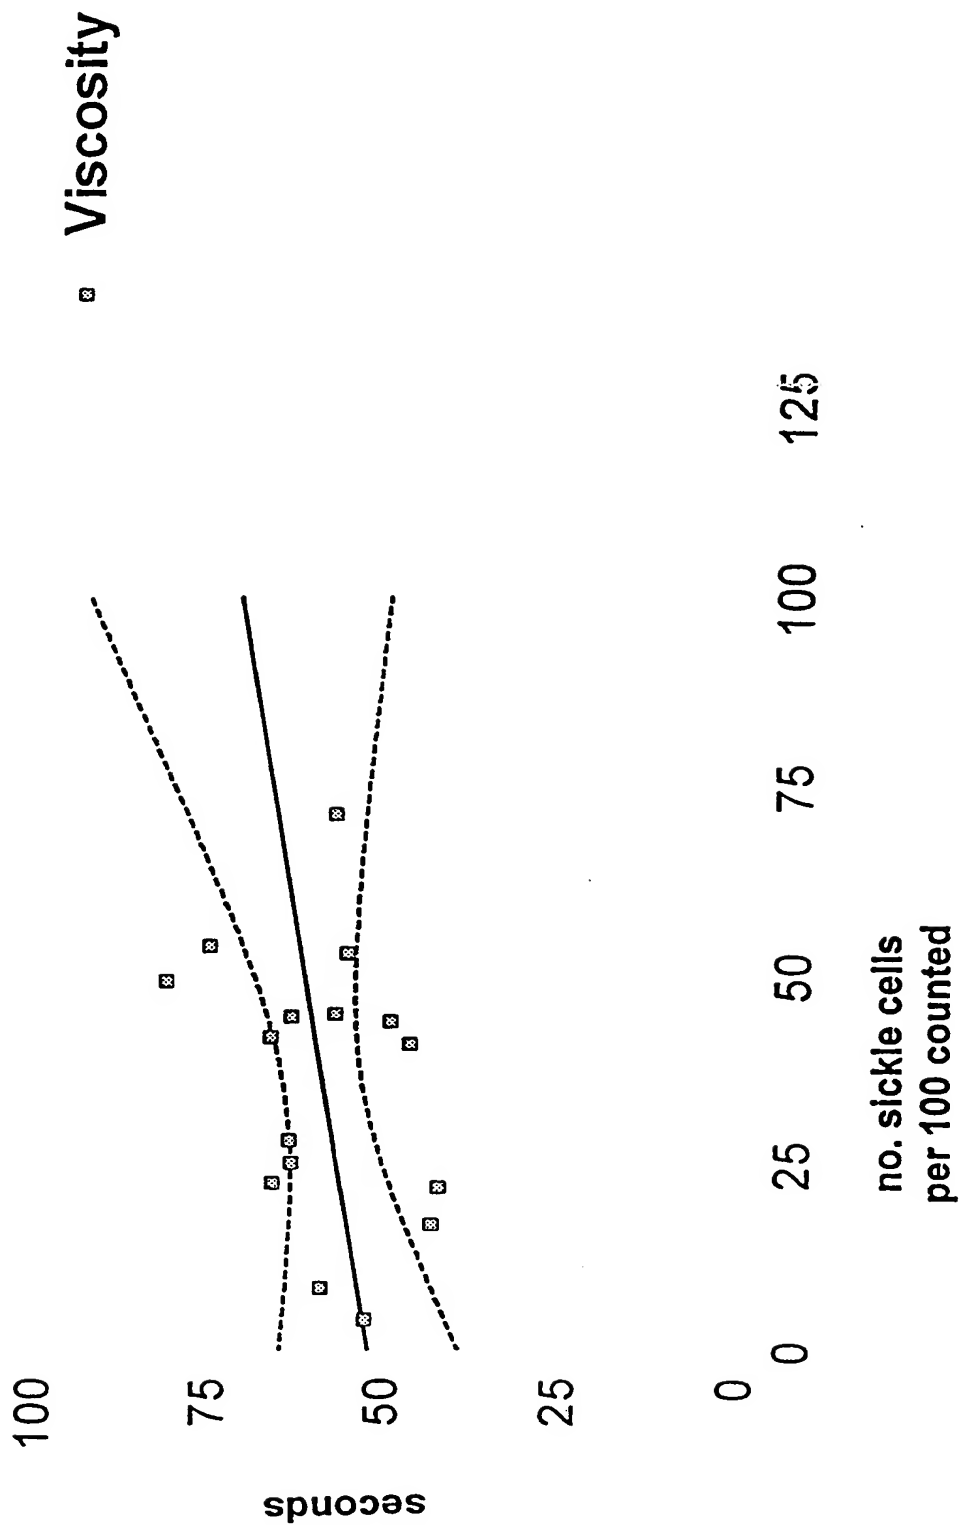


Fig. 3